



Multi-Spot Cartridge

**15 – 18 – 22 & 25**

**NOTE!** The laser operator and all staff in the laser treatment room should wear protective eyewear.

Hair type	Wave-length (nm)	Skin type	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Skin type	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Skin type	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	ICD (Pre/Delay/Post)			
<b>Fine</b> (Upper lip)	<b>755</b>	<b>I &amp; II</b>	<b>15</b>	1-2	10-14	<b>III</b>	<b>15</b>	3	12-15	<b>IV</b>	<b>15</b>	5	6-10	<b>20/10/0</b>			
			<b>18</b>		8-12		<b>18</b>		10-12		<b>18</b>		5-8				
			<b>22</b>		6-10		<b>22</b>		6-8		<b>22</b>		4-6				
<b>Medium</b> (Arms, Legs)			<b>15</b>	3	18-22		<b>III</b>	<b>15</b>	5		10-13	<b>IV</b>	<b>15</b>		5	8-12	<b>20/10/0</b>
			<b>18</b>		14-18			<b>18</b>			9-12		<b>18</b>			6-10	
			<b>22</b>		12-16			<b>22</b>			8-10		<b>22</b>			5-8	
<b>Coarse</b> (Beard, Axillary, Bikini line)			<b>25</b>	3	8-10		<b>III</b>	<b>25</b>	5		6-8	<b>IV</b>	<b>25</b>		10	4-6	<b>20/10/0</b>
			<b>15</b>		12-16			<b>15</b>			6-9		<b>15</b>			8-10	
			<b>18</b>		10-16			<b>18</b>			5-8		<b>18</b>			7-9	
<b>Coarse</b> (Beard, Axillary, Bikini line)	<b>22</b>	3	6-12	<b>III</b>	<b>22</b>	5	4-7	<b>IV</b>	<b>22</b>	10	6-8	<b>20/10/0</b>					

<b>Fine</b> (Upper lip)	<b>1064</b>	<b>III</b>	<b>15</b>	3	20-26	<b>IV</b>	<b>15</b>	5	12-18	<b>V &amp; VI</b>	<b>15</b>	5-12	8-14	<b>20/10/0</b>			
			<b>18</b>		18-22		<b>18</b>		8-12		<b>18</b>		6-12				
			<b>22</b>		14-18		<b>22</b>		6-8		<b>22</b>		5-10				
<b>Medium</b> (Arms, Legs)			<b>15</b>	5	18-22		<b>IV</b>	<b>15</b>	5		16-24	<b>V &amp; VI</b>	<b>15</b>		12-20	8-12	<b>20/10/0</b>
			<b>18</b>		16-20			<b>18</b>			14-20		<b>18</b>			8-10	
			<b>22</b>		12-16			<b>22</b>			7-16		<b>22</b>			4-10	
<b>Coarse</b> (Beard, Axillary, Bikini line)			<b>25</b>	5	10-14		<b>IV</b>	<b>25</b>	10-20		6-14	<b>V &amp; VI</b>	<b>25</b>		20	3~	<b>20/10/0</b>
			<b>15</b>		14-20			<b>15</b>			14-20		<b>15</b>			6-10	
			<b>18</b>		12-18			<b>18</b>			13-18		<b>18</b>			4-6	
<b>Coarse</b> (Beard, Axillary, Bikini line)	<b>22</b>	5	10-16	<b>IV</b>	<b>22</b>	10-20	10-16	<b>V &amp; VI</b>	<b>22</b>	20	3~	<b>20/10/0</b>					

**❖ Hair Removal**

✓ **IntelliTrak**  May utilize IntelliTrak mode.

- **Endpoint:** Perifollicular edema, mild erythema

- **Procedure:** Shave before the procedure to avoid energy waste and excessive skin reactions like burns. Perform a test spot for an appropriate skin response. In case of excessive skin reaction, decrease fluence by 2 J/cm<sup>2</sup>, then adjust pulse duration.

- **Wavelength:** **755 nm** – Lighter skin / Finer hair / Light hair color  
(The use of 755 nm to skin type IV requires a test spot before treatment.)
- **1064 nm** – Darker skin / Thicker hair / Dark hair color
- **Pulse width:** **Short** – Finer hair / Lighter skin  
**Long** – Thicker hair / Darker skin
- **Fluence:** **High** – Lighter hair color / Lower hair density / Smaller spot size  
**Low** – Darker hair color / Higher hair density / Bigger spot size

- **Post care:** Apply cold compress or Ice pack cooling and hydrocortisone (~1%) to avoid any possible side effects.

- **Treatment interval:** 4-6 weeks for the face, and 6-8 weeks for all other areas



Multi-Spot Cartridge

**15 – 18 – 22 & 25****NOTE!** The laser operator and all staff in the laser treatment room should wear protective eyewear.**Expert's Recommendation**

Protocols from experts that are proven to be effective.

Indication	Step	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
Dual Hair Removal	1	1064			Lower the fluence by 2-3 steps than the usual parameter.		20/10/0	1	4-6	3-5
	2	755						Lower the fluence by 2-3 steps than the usual parameter.		

**❖ Dual Hair Removal**

Effectively target various types of hair (thickness, depth, and color) using both wavelengths in one procedure.

**- Endpoint: Perifollicular edema, mild erythema****- Procedure:** Lower the fluence by 2-3 J/cm<sup>2</sup> than the usual parameter when performing multiple passes. Perform both steps 1 and 2 in one procedure.

Indication	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
Alex Peel (Fine hair)	755	18	3	6~	2~	10/10/5	1	4-6	3-5

**❖ Alex Peel**

Effectively target fine soft hair all over the face, brighten the skin tone, and prevent inflammation. This could be combined with Ice Nevus Removal, Alex Toning or InnerLift Mild treatment.

**- Endpoint: Mild erythema**



Multi-Spot Cartridge

8 – 10 – 12

**NOTE!** The laser operator and all staff in the laser treatment room should wear protective eyewear.

Indication	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
Facial Flushing	1064	12	40-60	20-26	2~	20/10/0	2-3	3-4	3-5
Active Acne	1064	8	20	20	2-3	0/0/10	1-3	1-2	5
Rosacea	755	8	12	18-24	1	10/10/10	1	4-12	3-5

**❖ Vascular Lesion****- Endpoint: Erythema****- Post care:** Apply cold compress or ice pack cooling, and hydrocortisone (~1%) to lower the chance of side effects.**Expert's Recommendation**

Protocols from experts that are proven to be effective.

✓  May utilize Skin Temp mode.

Indication	Step	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
Clear Flush (Facial flushing)	*1 (Optional)	755	8	3	14-18	3	OFF	1-2	2 (3-4 weeks for children)	6
	2			5	14-18	3		1-2		
	3			12	14-18	3		1-2		
	4	1064	8	20	20~	3	OFF	1-2		
	5			30	30~	3		1-2		

**❖ Clear Flush**

Normalize facial flushing and minimize recurrence through dermal remodeling using both 755 nm and 1064 nm.

**- Endpoint: Erythema****- Procedure:** Check the temperature of the skin during the treatment using **Skin Temp mode** or skin palpation.

During the treatment, ice pack cooling could be applied to prevent excessive heat accumulation.

**- Note:** For darker skin type patients, step 1 could be skipped.**- Post care:** Apply cold compress or ice pack cooling, and hydrocortisone (~1%).

Indication	Step	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
Clear Rosacea * Paper published	1	755	10	12	30~	2-3	20/10/0	1-2	4	3-5
	2	1064	10	0.5	3~	10	OFF	6		

**❖ Clear Rosacea (Paper published)**

「 Prospective Comparison of Dual Wavelength Long-Pulsed 755-nm Alexandrite/1,064-nm Neodymium:Yttrium-Aluminum-Garnet Laser versus 585-nm Pulsed Dye Laser Treatment for Rosacea 」

This parameter proved effectivity and safety with a similar clinical effect to PDL.

**- Endpoint: Mild erythema****- Procedure:** Check the temperature of the skin during the treatment using **Skin Temp mode** or skin palpation.

Perform both steps 1 and 2 in one procedure.

**- Post care:** Apply cold compress or ice pack cooling, and hydrocortisone (~1%).



Multi-Spot Cartridge

8 – 10 – 12

**NOTE!** The laser operator and all staff in the laser treatment room should wear protective eyewear.

Indication	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
<b>Alex Toning</b> (Melasma, PIH, Uneven skin tone)	755	10	0.3	3-4	5-10	OFF	3-5	1-2	5-10

**❖ Alex Toning**

Gentle and safe pigment bleaching technique to treat pigmented lesions across the entire face.

- **Endpoint:** Mild erythema
- **Post care:** Soothe and moisturize the skin.

**Expert's Recommendation**

Protocols from experts that are proven to be effective.

Indication	Step	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
<b>Brightening for Man</b>	1	755	8	0.7	9	5~	OFF	1-2	2	5
	2	755	8	0.3	5.5	5~		2		

**❖ Brightening for Man**

The first step is effective facial fine hair removal, and the second step is to brighten the dull skin tone.

- **Endpoint:** Perifollicular edema, mild erythema
- **Procedure:** Perform both steps 1 and 2 in one procedure.
- **Post care:** Apply cold compress or Ice pack cooling, and hydrocortisone (~1%).



Multi-Spot Cartridge

16 – 20 – 25


**NOTE!** The laser operator and all staff in the laser treatment room should wear protective eyewear.

Indication	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
InnerLift Mild	1064	16	0.3	2~	5-10	OFF	5-8	1-2	5-10
InnerLift Moderate	1064	16	20	14~	2~	10/10/0	3-5	1-2	5~
InnerLift Advanced	1064	16	50-60	22-26	2	20/10/0	2-3	2-3	3~

**❖ InnerLift Mild**

Skin rejuvenation technique that improves skin texture and fine wrinkles.

- **Endpoint:** Mild warming sensation, mild erythema
- **Procedure:** Control the number of passes by observing the skin reaction.
- **Post care:** Apply cold compress, skin soothing and moisturizing.



✓ May utilize Skin Temp mode.

**❖ InnerLift Moderate**

A laser facelift that does not require anesthesia. It improves the appearance of fine wrinkles and facial flushing by enhancing skin rejuvenation through dermal collagen remodeling. Improved skin elasticity is visible on an average of one month after the procedure.

- **Endpoint:** Moderate warming sensation, mild erythema
- **Procedure:** Consider the general direction of the face lift by targeting the center of the face toward the outer portions. ICD mode could be skipped in this procedure.
- **Post care:** Apply cold compress, skin soothing and moisturizing.

**❖ InnerLift Advanced**

Traditional skin rejuvenation technique that uses long pulse width and high fluence. It effectively induces collagen remodeling, tightens the pores, and improves the appearance of wrinkles.

- **Endpoint:** Strong warming sensation, erythema, mild edema
- **Procedure:** The laser irradiates from the center of the face toward the outer portions. Turn on the **Skin Temp mode** to observe skin reaction and to reach ~47°C. Apply cooling after the treatment.
- **Post care:** Apply cold compress, skin soothing and moisturizing.

**➤ Example of Combination Treatment:****1) INNERLIFT COMBINATION**

: A combination treatment that effectively improves skin tone, texture, laxity, pores, and wrinkles.



STEP ① **InnerLift Mild**  
2-3 passes to the entire face

STEP ② **InnerLift Moderate**  
2-3 passes to the perinasal area

STEP ③ **InnerLift Advanced**  
2-3 passes to the jawline

**2) Melasma Treatment & InnerLift Mild**

: Improve dermal condition to prevent recurrence of melasma.

**3) Facial Flushing Treatment & InnerLift Mild**

: Normalize dilated blood vessels and induce dermal remodeling.

**4) Blackhead Treatment & InnerLift Moderate**

: Tighten pores after extrusion and rejuvenate the skin.



Multi-Spot Cartridge

16 – 20 – 25

**NOTE!** The laser operator and all staff in the laser treatment room should wear protective eyewear.**Expert's Recommendation**

Protocols from experts that are proven to be effective.



✓ May utilize Skin Temp mode.

Indication	Step	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
CLA-Rejuvenation	1	755	25	0.3	1.5-1.7	5-10	OFF	3	2	5
	2			0.5	1.5-2	5-10		2-3		
	3			0.7	1.5-2	5~		2-3		
	4	1064	25	0.3	1.5-2	5-10	OFF	3		
	5			0.5	1.5-2	5-10		1-2		
	6			0.7	1.5-2	5~		1-2		

**❖ CLA-Rejuvenation**

Effective skin rejuvenation using 6 different steps of pulse widths shorter than 1 ms. Skin overproduces melanin pigments when exposed to UV light. The 755 nm reduces the amount of UV transmission and improves the epidermal condition. And the 1064 nm improves the dermal condition to maintain the effect and prevents a melasma recurrence.

- **Endpoint:** Erythema, warming sensation
- **Procedure:** Control the number of passes and overlapping by observing the skin reaction.
- **Post care:** Apply cold compress or ice pack cooling in between the treatment, skin-soothing, and moisturizing.

Indication	Step	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
CLA-Lift	1	755	25	3	1.6~	5~	OFF	3-5	2	5
	2			12	1.8~	5~		2-3		
	3	1064	25	3	1.7~	5~	OFF	3		
	4			12	1.8~	5~		2-3		

**❖ CLA-Lift**

Effective laser facelift treatment with the use of a 25 mm spot size that penetrates deep in the skin. 755 nm improves the epidermal condition and skin texture. And the 1064 nm induces collagen remodeling and increases skin elasticity.

- **Endpoint:** Erythema
- **Procedure:** Cool in between the treatment. Control the number of passes and overlapping by observing the reaction.
- **Post care:** Apply cold compress, skin-soothing, and moisturizing.

Indication	Step	Wavelength (nm)	Spot size (mm)	Pulse width (ms)	Fluence (J/cm <sup>2</sup> )	Pulse rate (Hz)	ICD (Pre/Delay/Post)	Pass	Interval (week)	Session
C-Toning Rejuvenation	1	755	16	5 [C-Toning]	5	5	OFF	1-2	1-2	5
	2	1064	16	5 [C-Toning]	5-7	5-10	OFF	3		

**❖ C-Toning Rejuvenation**

Target pigments in the basal layer using a 16 mm spot size and C-Toning mode. This effectively improves melanosomes that react from 0.1-5 ms and gradually heats up the dermis to induce dermal remodeling.

- **Endpoint:** Mild erythema
- **Procedure:** Control the number of passes and overlapping by observing the skin reaction.

# Operation & Maintenance



## GUI

### Wavelength

Alexandrite 755 nm or Nd:YAG 1064 nm is selectable. Press 2 seconds to change.

### Shot Count

The number of laser shots emitted.

### Pulse Width

Time duration of one laser shot (0.1-300 ms).

### C-Toning Mode

A macropulse consisting of 0.1 ms sub-pulses (3/5/10 ms).

### Operating Switch

Laser radiation control. Select either Finger or Foot switch.

### ICD

**[Intelligent Cooling Device]**  
Select whether to use the cooling function (ON/OFF). When the function is ON adjust (Pre/Delay/Post) time.

### Standby / Ready

When changed to Ready, laser emission is possible.

### Setup

Check total shot count, parameter history, sound volume, etc.

### Memory

Press whether to enter the save mode to save the parameters or load the saved parameters.

### Parameter Capture

Save the parameter displayed on the screen.

### Spot Size

The diameter of the laser beam (mm).

### Fluence

Energy per unit area (J/cm<sup>2</sup>).

### Pulse Rate


The number of the laser shots per second (Hz).

### Overlap Percentage

When IntelliTrak mode is ON, Select overlap percentage (-15/0/18/30/50%).

### IntelliTrak Mode

This Mode is only available when IntelliTrak tip is connected (ON/OFF).

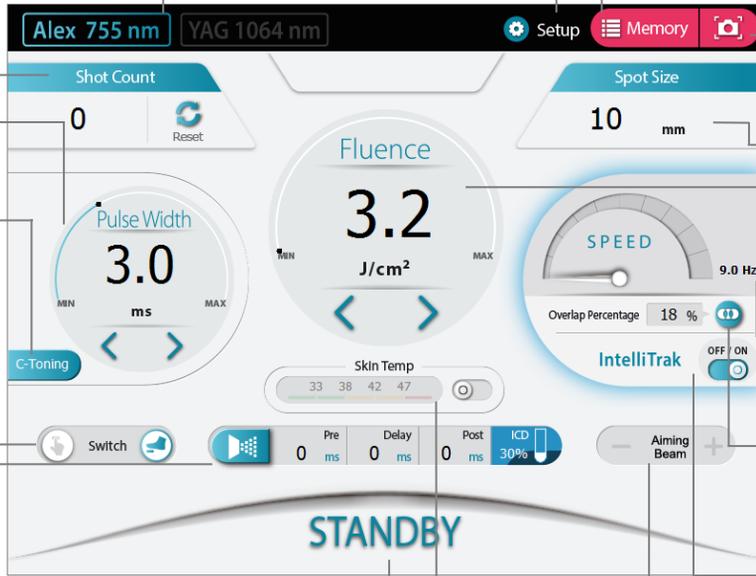

## IntelliTrak Mode



with IntelliTrak Tip

### ❖ Speed Gauge Bar



**Green**  
Less than 75% of max. Hz




**Yellow**  
75% to 100% of max. Hz



**Red**  
100% or more of max. Hz

- In IntelliTrak mode, the pulse rate is displayed on the speedometer with colors of green, yellow, or red.
- If the actual handling speed is faster than the pulse rate, the GUI and the LED color of the handpiece turn to **Red**, and laser emission automatically stops.

### ❖ Overlap Setting (-15, 0, 18, 30, and 50%)

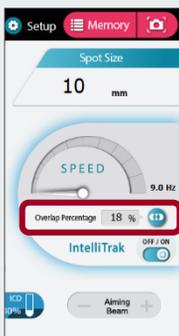

- Overlap setting function enables rapid and consistent treatment on the large area.
- 18% is the most ideal for hair removal.** More overlap is recommended for the lighter skin type and lesser for the darker skin type.

## Skin Temperature Mode

### ❖ Real-time Skin Temperature Sensor



1st : ~33°C    1st : ~42°C    1st : 47°C~  
2nd : ~38°C    2nd : ~47°C


- \* Live skin temperature check through colors of **Green**, **Yellow**, and **Red**.
- \* Temperature range is adjustable from **Setup**.

- The Skin Temperature function allows the user to visually check whether the temperature of the skin surface is excessively increased due to laser treatment.
- When the Skin Temp mode is on, it is usable in both the **READY** and **STANDBY** status.
- When the color of the Skin Temp bar from GUI and the LED color of the handpiece turn red, the device switches to **STANDBY** mode with a beeping sound, and laser emission becomes disabled.
- The Skin Temp mode is automatically deactivated if the ICD cooling function of the device is turned on.


# Operation & Maintenance

## Memory & Capture

### Memory



- Press 'Memory' to save frequently used parameter.

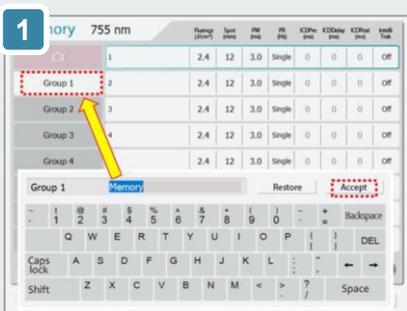

- Press 'Rename' button to enter group name and treatment name using a pop-up keyboard.
- Press 'Accept' to save.




- Press 'Modify' to input parameters then press 'Accept'.
- In case saving current parameter, press 'Import' icon to call the protocol then press 'Accept' to save.



- Select the saved memory.
- Then treatment name appears on the top of the GUI, and parameters are automatically set.

### Capture



- Press 'Capture' to save parameter displayed on GUI.
- Press 'Memory' to view captured history.



- A total of 8 parameters are savable in Capture. When the list is filled, the oldest parameter is deleted and the newest one is saved.





- Press 'Rename' located on the bottom to enter a treatment name using a pop-up keyboard.
- Press 'Accept' to save.



- The capture group can be moved to the top or bottom of the group list, by clicking the buttons located at the bottom.

## ICD

- Activate ICD mode by pressing 'Spray' button.

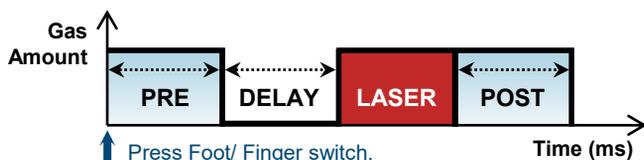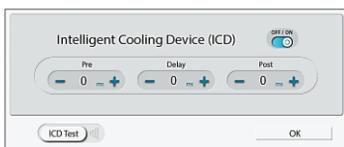

- **PRE** ICD gas emitting before laser irradiation
- **DELAY** Time interval between pre and post emitting
- **POST** ICD gas emitting after laser irradiation

## How to Replace

- Press the gas amount button  to check the percentage of remained ICD gas.
- Whenever a new ICD canister is replaced, set the initial value of ICD amount to 100%.

### 1 Caution (Check 00 00 00 08)


CHK 04 : Replace ICD canister.



- When "Replace" message pops up, open the cap and remove the old ICD canister.

### 2 Caution (Check 00 00 00 04)

CHK 03 : Insert ICD canister.  
... (Multiple system errors detected)



- When "Insert" message pops up, insert a new canister.
- **[Note]** ICD mode should be ON.

### 3




- Press the cap by turning right to fix the canister.



**[Note]** Once replaced, press 'ICD Test' button 3-5 times to remove probable gas bubbles stuck into the fiber.

## Handpiece

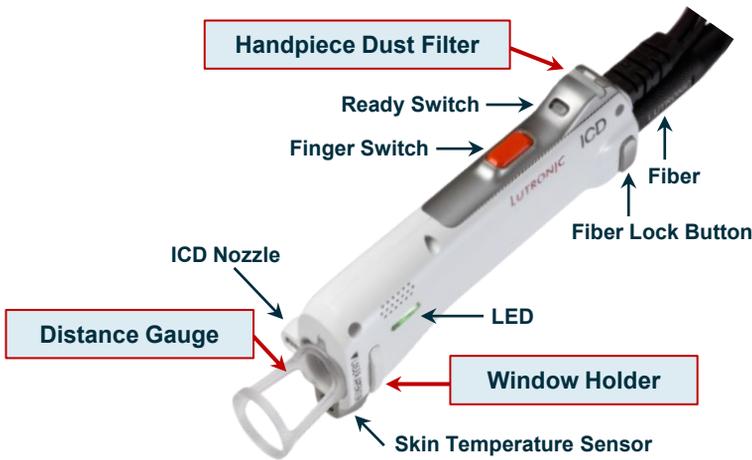

\*  : Always check its cleanliness before the treatment.



- To connect the multi-spot cartridge, mount the handpiece securely into the holder.
- Keep the storage box closed to protect accessories from dust.

**[Note!]** Do not bend or wind the optical fiber to a radius of less than 30 cm.

## How to Connect

### Multi-Spot Cartridge



- Select appropriate multi-spot cartridge according to the lesion.
- Attach it to the optical fiber.
- Insert the cartridge with fiber into the handpiece.

### Distance Gauge



- Select appropriate distance gauge.
- Attach the distance gauge in front of the handpiece by matching the groove or port.

\* There is no groove on 'I Tip.'



### Replaceable Window



- Insert the window into the slot above Laser Aperture.
- Window is replaceable from the storage box.

## Maintenance

### Handpiece Window

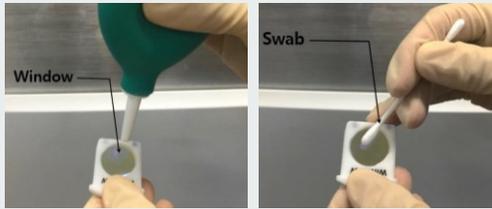

- Pull out the window from the handpiece and check its cleanliness.
- If there is any debris, remove it using an air dust blower or glasses cloth.
- For sticky dust, use a cotton swab soaked with ethanol (70% or higher).

**[Note!]** The window must always be inserted at a correct angle to avoid window damage or break.

- In case of a damaged window, gently push it from the holder to remove and replace it with a new window.

### Distance Gauge



All Tips



IntelliTrak Tip

- Keep the distance gauge in place or separate from the handpiece.
- Clean the surface with a cotton swab soaked in ethanol (70% or higher) before and after treatment (especially after hair removal).
- For the IntelliTrak tip, separate the roller and clean it with ethanol.

### Handpiece Dust Filter



- Pull out the filter from the top of the handpiece.
- Gently rub off the dust with a towel first, then spray water.
- Dry the filter in a shady place, then insert it into the handpiece.

**[Note!]** Check the filter once a month to see if it is dirty.

### Device Dust Filter



- Remove the dust filter from the frontal side of the body by grasping both ends and pulling it downwards.
- Gently wipe the dust from the surface with a towel first, then remove the remaining dust by spraying cold water onto the filter.
- Let the cleaned dust filter dry completely in a shady, well-ventilated place and then couple it back to the device.

**[Note!]** Check the device filter once in 3 months.



▲ After 3 months    ▲ After 6 months

## Patient Post-Treatment Care

- Please do not use cosmetics with retinol or AHA for 48 hours.
- Please do not use hydrocortisone for more than 2 days without a doctor's prescription.
- Please do not use an exfoliator or scrub to the treated area for a week after treatment.
- Please do not take the sauna for a week after treatment.
- Please do not pluck hair after hair removal treatment to avoid folliculitis caused due to inflammation.
- Apply a UVA/B sunblock of more than SPF30, PA++ for at least 30 days after treatment.
- Please inform the doctor about the medications you are currently taking.
- Apply a cooling pack to the excessive erythema affected by the treatment for more than 20 minutes.

**For more information, please contact your physician at the address below.**

